

**SMC™ : an alternative to other technologies  
for development of immunogenicity assay  
for cytokines ADA**

**EIP Lisbon– 17-19 February 2020  
Eric Guillemare**




**Translational Medicine and Early Development  
Biomarkers & Clinical Bioanalysis**

# ADA Assay method : classical bridging format

Classical format : bridged complex ADA-Drug in solution  
Drug labeled with biotin or SulfoTag

**Drug** : large molecule i.e. therapeutic antibody

- MW ADA ~ MW drug ~ 150 kDa
- Diversity of epitopes recognized by ADA
- Diversity of sites for drug labeling without downgrading functionality

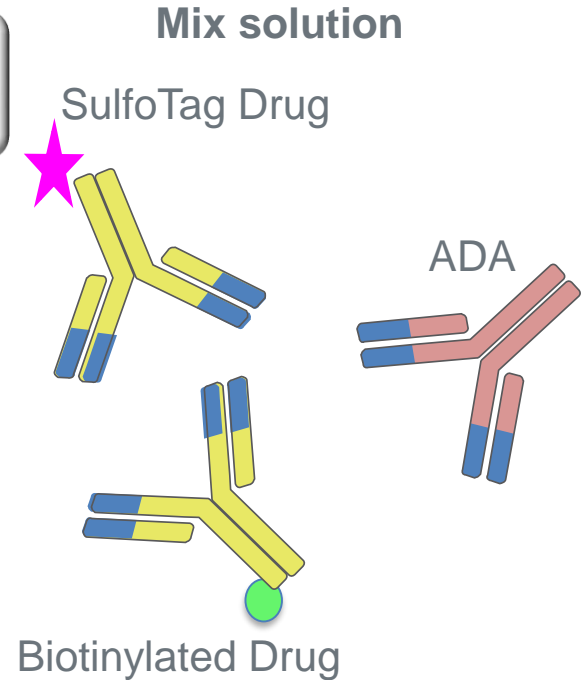

# Assay method for ADA detection directed against cytokines: new project for a clinical study

Three cytokines in human samples with LOW/MEDIUM risks of immunogenicity :  
CytA, CytB and CytC

Need to develop assay three methods for ADA detection



## Difficulties related to cytokines :

- MW ADA ~ 150 kDa
- MW drug ~ 10-20 kDa
- Low number of epitopes recognized by ADA
- drug labeling risks to downgrade functionality
- Behavior of cytokines:

CytA : contains a membrane subunit

CytB: risk of aggregation or fixation to plasma protein

CytC: is a heterodimer

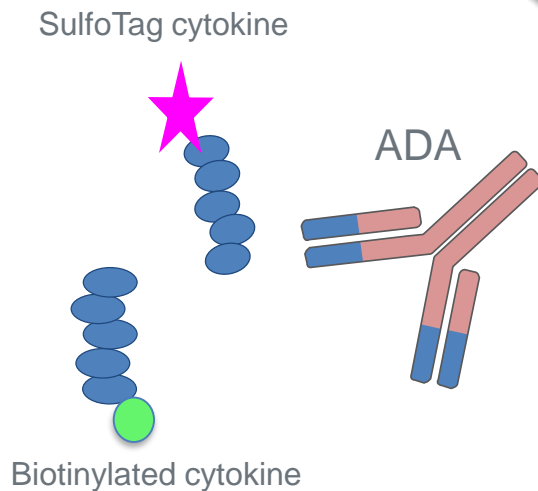


# Assay method for ADA detection directed against cytokines: classical bridging format

Mix solution

Format : bridged complex ADA-Drug in solution  
Drug : cytokine labeled with biotin or SulfoTag


SulfoTag cytokine

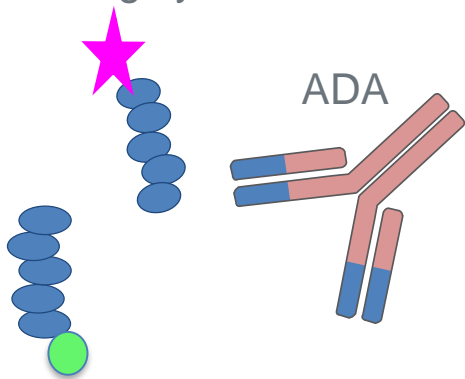

Biotinylated cytokine

- Need to adapt rate of labeling on each cytokine
- Need to optimize quantity of labeled cytokines in Mix solution

# Assay method for ADA detection directed against cytokines: classical bridging format using Electrochimiluminescence (ECL)

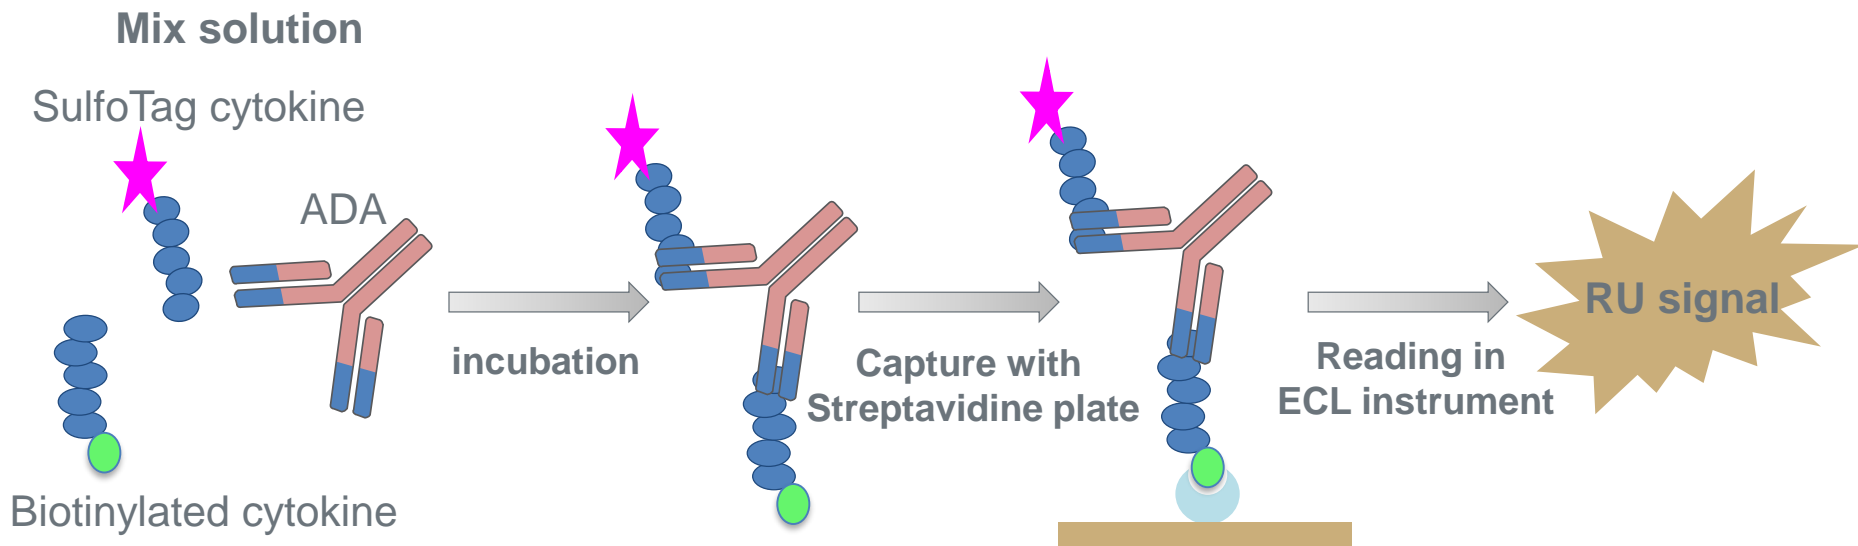


# Method developments of ADA against cytokine using ECL

Results for three cytokines using ECL and after optimization !

## Reagents :

- **Matrix** : Human plasma
- **Standards** : ADA obtained by injection of cytokines CytA, CytB or CytC in rabbit
- **Low PC** : spiked at the expected sensitivity: 0.1  $\mu\text{g/mL}$  ADA

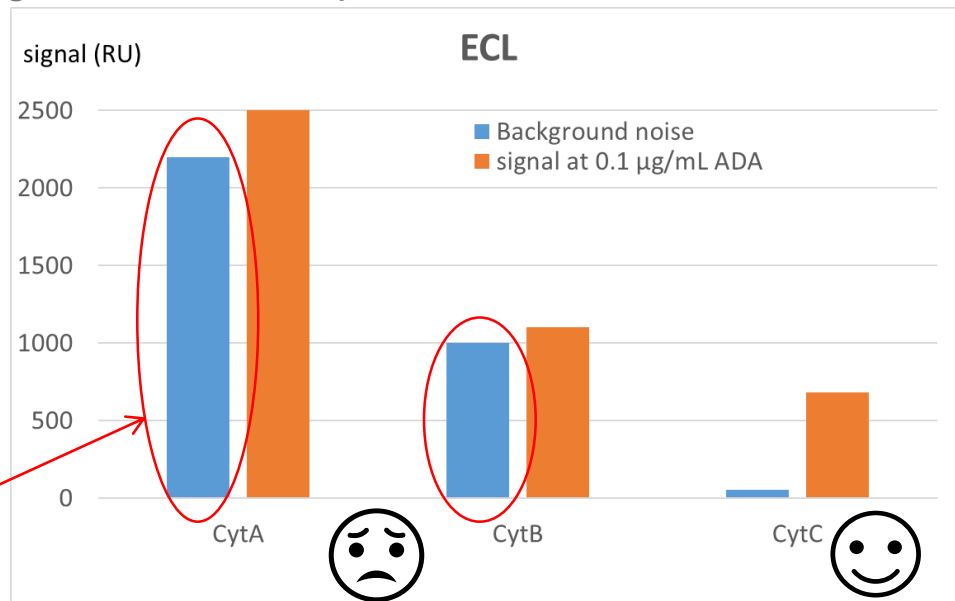


- For CytA and CytB : in spite of the optimization of the experimental conditions, the background signal was still too strong
- For CytC : sensitivity at 0.1  $\mu\text{g/mL}$

Need to test another technology : **SMC™**

# Single Molecule Counting (SMC™) technology

Merck's propriety Single Molecule Counting (SMC™) technology :

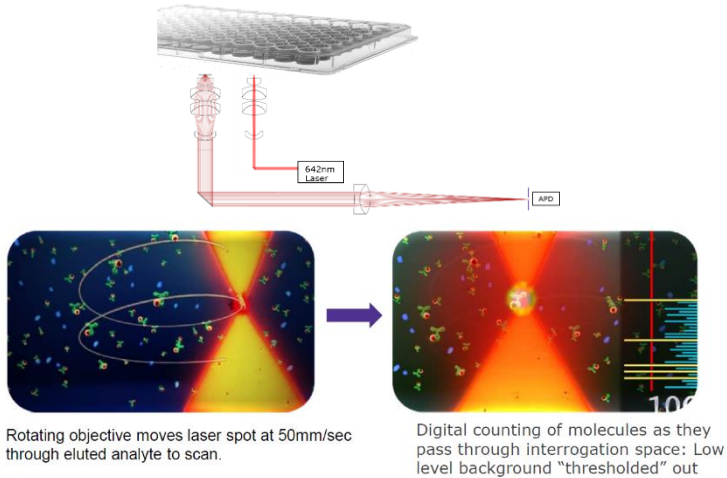


- Rotating objective scans laser spot through analyte.
- 642 nm laser focused through plate
- Single fluorochromes excite and emit fluorescence : labeling with AlexaFluor 647
- Signal output = Response signal

SMC™ Immunogenicity Assay Development Kit (Cat. No. 03-0175-00) has been available since last year

- Need feedback for ADA
- Assessment of SMC™ for development ADA methods for CytA, CytB and CytC using SMCxPro
- **Expected benefit:** Decrease background and a sensitivity at 0.1 µg/mL

# Method development of ADA using SMC™ technology

## Bridging format

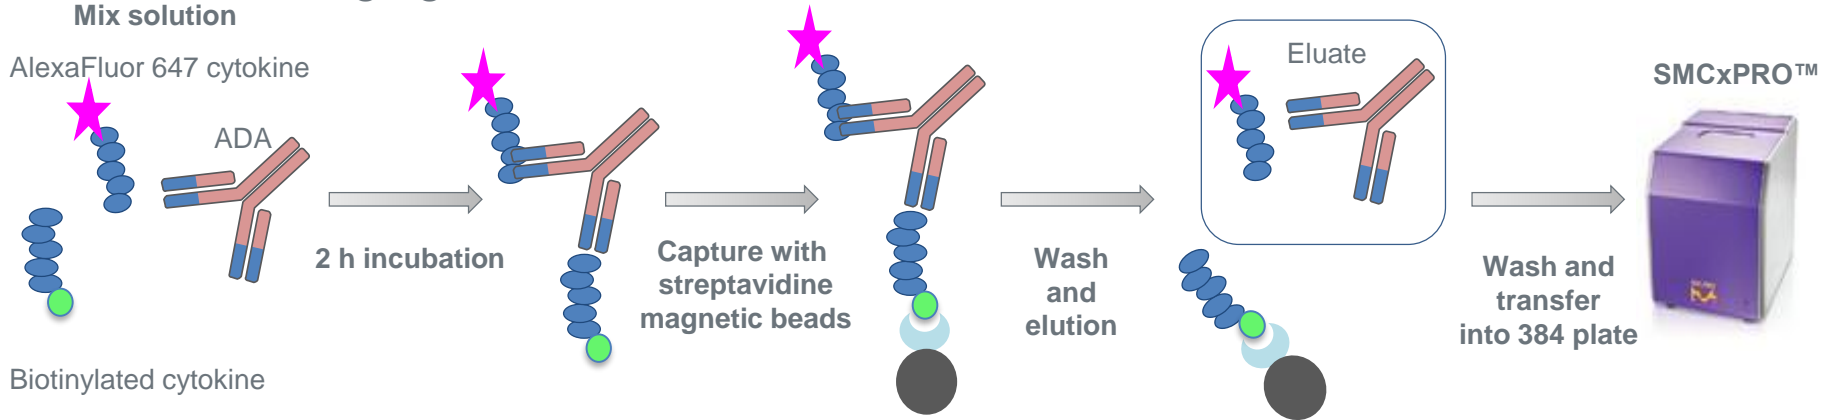

### Positive elements:


- Capture with magnetic beads → best capture/presentation of epitope, washing efficiency
- Elution step → decrease non-specific signal
- SMC™ is described as an ultrasensitive technology for PK and BM purpose, but there are no publications about ADA.



# Method developments of ADA against cytokine with SMC™

## Results for three cytokines using SMC™

- **Matrix** : Human plasma
- **Standard** : ADA obtained by injection of cytokines CytA, CytB or CytC in rabbit
- **Low PC** : spiked at the expected sensitivity: 0.1 µg/mL ADA

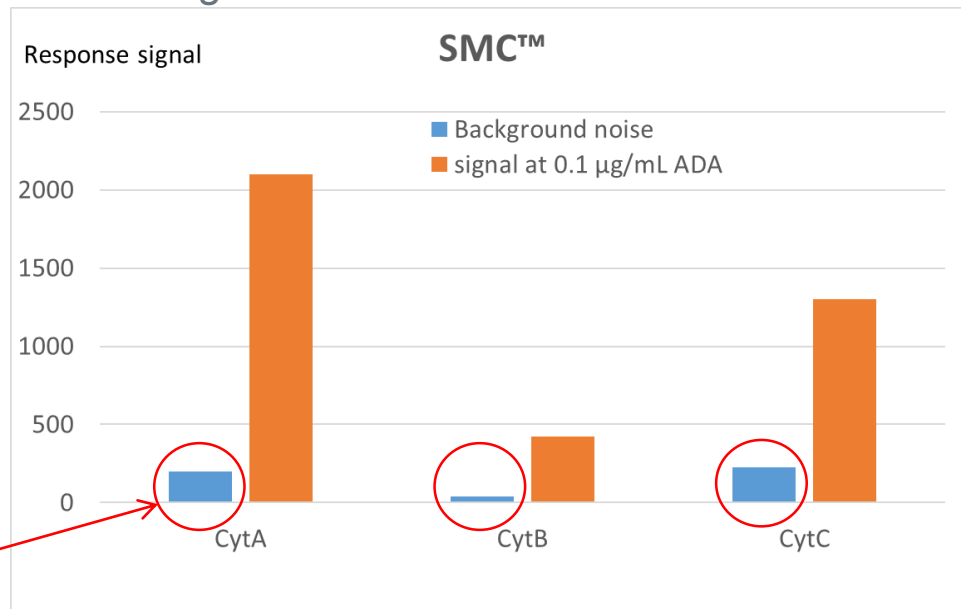

Low background signal

- Low background noise signal
- Sensitivity at 0.1 µg/mL



ADA method developments on  
**CytA, CytB and CytC** can be done with SMC™


# Method developments of ADA against CytA with SMC™

Instrument saturation at 20 000 response signal




Need to optimize conditions in order to avoid Signal saturation:

- Decrease quantity of labeled cytokines : be careful to hook effect !
- Decrease MRD

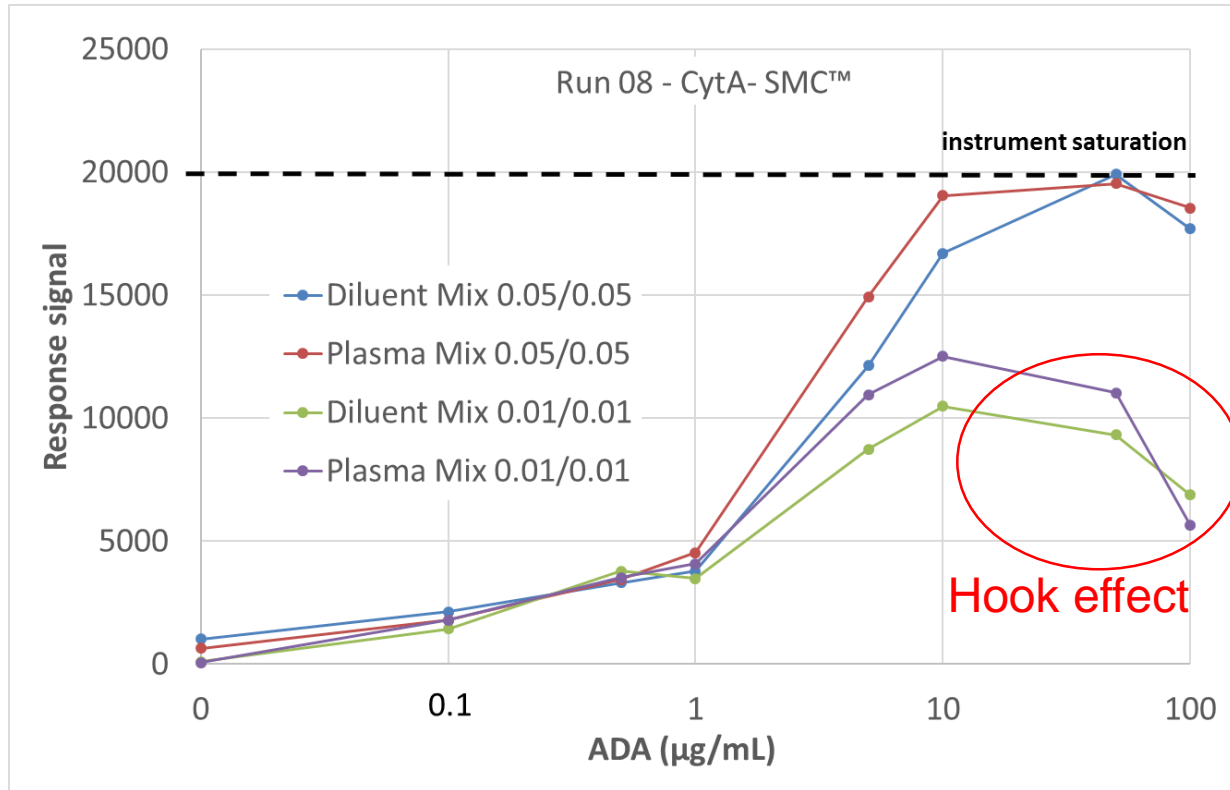

# Method developments of ADA against CytA with SMC™


- **Mix solution** : 0.025 and 0.05  $\mu\text{g/mL}$
- **Standard ADA** : 0.1 to 100  $\mu\text{g/mL}$
- **Matrix**: diluent or plasma
- **MRD** : 1/60
- **Final conditions** :  
MRD 1/60  
Mix 0.025  $\mu\text{g/mL}$  (labeled cytokines)

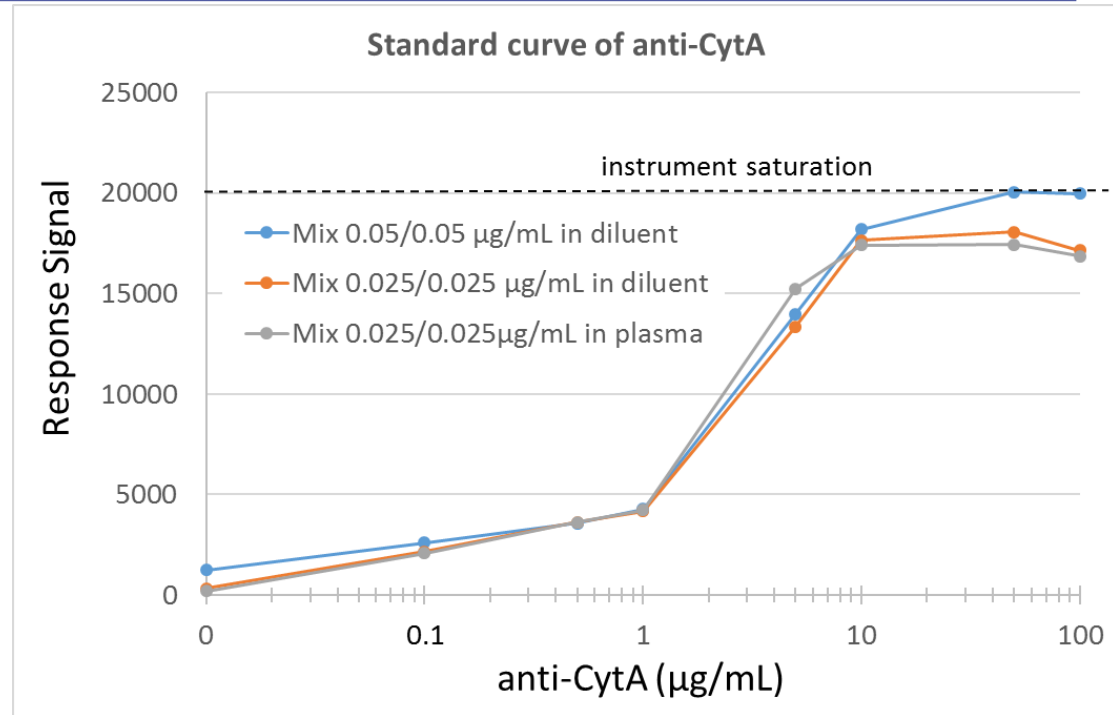

- Low background noise signal
- Sensitivity at 0.1  $\mu\text{g/mL}$
- No instrument saturation for high concentrations of ADA

# Estimation of cutpoint with SMC™

For a first estimation of cut-point, 40 healthy plasmas were analyzed in screening condition MIX 0.025 µg/mL and MRD 1/60

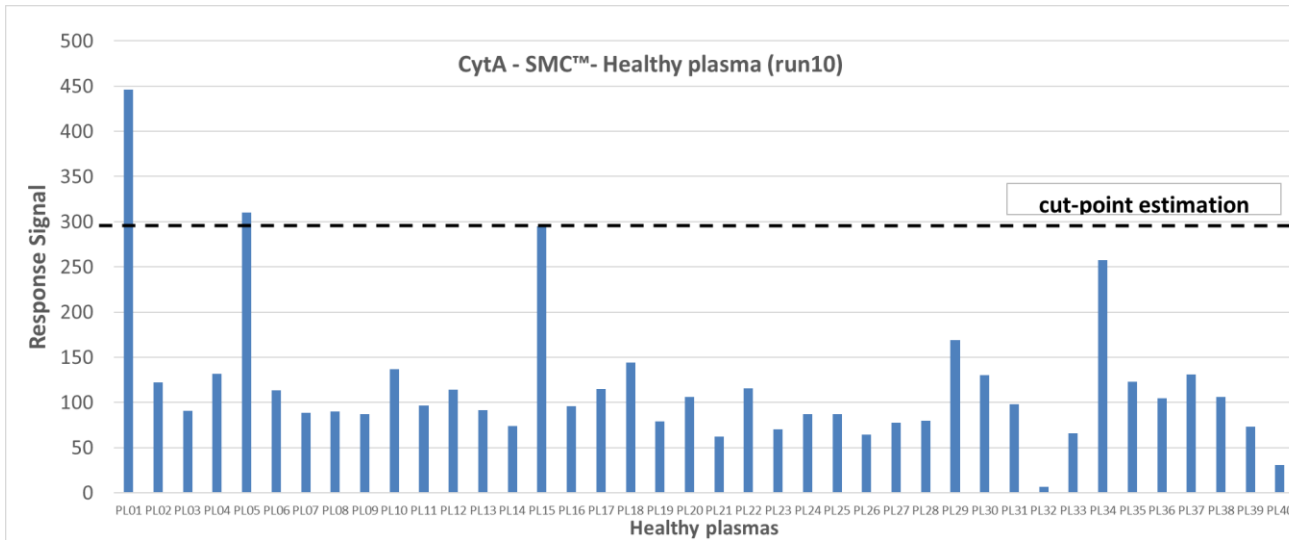

Estimation of Ncut-point at 1.34 and cut-point at 295 response signal (based on 95 percentile)


# Assessment of confirmation condition with SMC™

- **Confirmation test** : competition with CytA at 1, 3 and 10 µg/mL
- **Low PC** : 0.1 µg/mL standard ADA
- **High PC** : 10 µg/mL standard ADA



**3 and 10 µg/mL of CytA were sufficient to reach cut-point level**

Be careful: too high CytA quantity could be unbalance the complex ADA-labeled cytokine and act as protein effect.

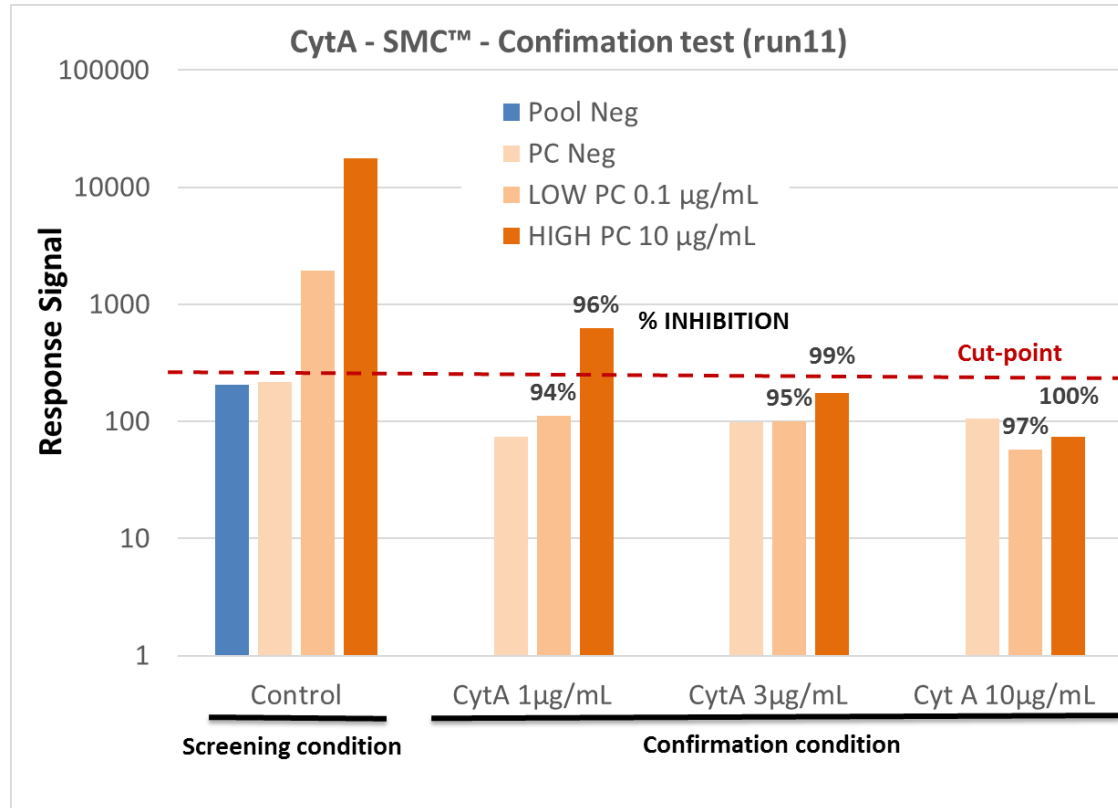

# Conclusions on these ADA methods

---

- Only CytC ADA method could be developed with ECL (low background signal only for this cytokine)
- SMC™ technology allows to decrease background signal and reach sensitivity at 0.1 µg/mL for CytA, CytB and CytC
- For CytA:
  - Experimental conditions optimized for screening and confirmation tests
  - Need to check free drug tolerance, specificity and titration process
  - Next step : validation of method

# Conclusions on SMC™ technology

SMC™ is an alternative to other technologies for development of immunogenicity assay

	Pros	Cons
<b>SMC™ technology</b>	Decrease background signal Increase sensitivity Magnetic beads allow to increase capture Reagents consumption can be reduced	require magnetic washer and robustness depends in part on the <b>wash step optimization</b>
<b>Productivity</b> (Number of samples per day for 1 equipment and 1 analyst)	around 40 samples / day more than 1 plate/day depending on magnetic washing equipment	
<b>SMC™ Reagent</b>	Immunogenicity Bead Based Assay Development Kit (967 €); possibility to buy buffers separately	
<b>Robustness</b>	yes but need to be validated for ADA method	
<b>LIMS interface</b>	yes	
<b>IQ - OQ availability</b>	yes	
<b>Availability in CRO</b>	not all CRO	
<b>Multiplex</b>		No multiplex

# THANK YOU

Acknowledgment:

L. Diouloufet, P. Juhue, N. Bremond, L. Vermet, O. Fedeli  
Sanofi Montpellier, France

And

Ludivine Grosjean , Daniel Garcia West  
Merck Millipore